


Chloroquine**Column:** N/A**Dimensions:** N/A**Order No:** N/A**Elution Type:** N/A**Eluent A:** Hexane/Dichloroethane/Ethanol-TFA (40:35:25) w/ ethanol-TFA (20:1)**Gradient** **Step No.** **Time (min)** **Pct A****Profile:** **1** 0 100**Flow Rate:** 1 mL/min**Col. Temp.:** ambient**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 346 nm (ambient)**ANALYTES:****1** Chloroquine

Retention Time: 14.95 min

2 Chloroquine

Retention Time: 16.51 min

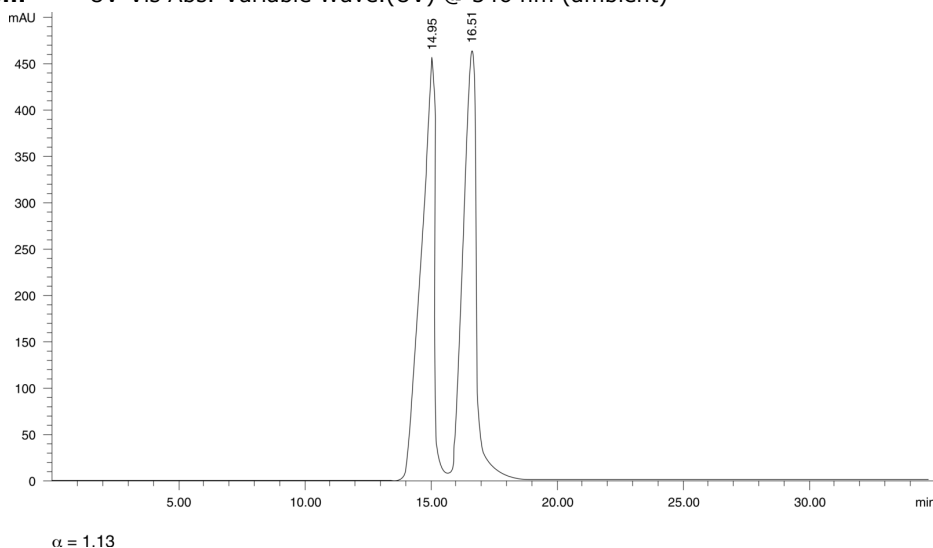