


6-MAM and Interferences by MSD on a ZB-5MSi**Column:** Zebtron[™] ZB-5MSi, GC Cap. Column 10 m x 0.18 mm x 0.18 μ m, Ea**Phase:** 5% Phenyl 95% Dimethylpolysiloxane**Dimensions:** 10 meters x 0.18 mm x 0.18 μ m**Order No:** 7CD-G018-08**Oven Profile:** 170 °C to 300 °C @ 20 °C/min**Carrier Gas:** Constant Flow Helium, 0.7 mL/min**Injection:** Split 10:1 1 μ L @ 260°C**Detection:** Mass Selective (MSD) (320°C)**Analyst Note:** Analytes are 24ppm derivatized with BSTFA
Sim ions:
(Quant ion*) D3-6-MAM (*402,403): 6-MAM (*399,400,340)**Products used in this application:****ANALYTES:**

- 1 Hydromorphone
- 2 Morphine
- 3 Norcodeine
- 4 Codeine
- 5 Hydrocodone
- 6 6-MAM-d3
- 7 6-MAM

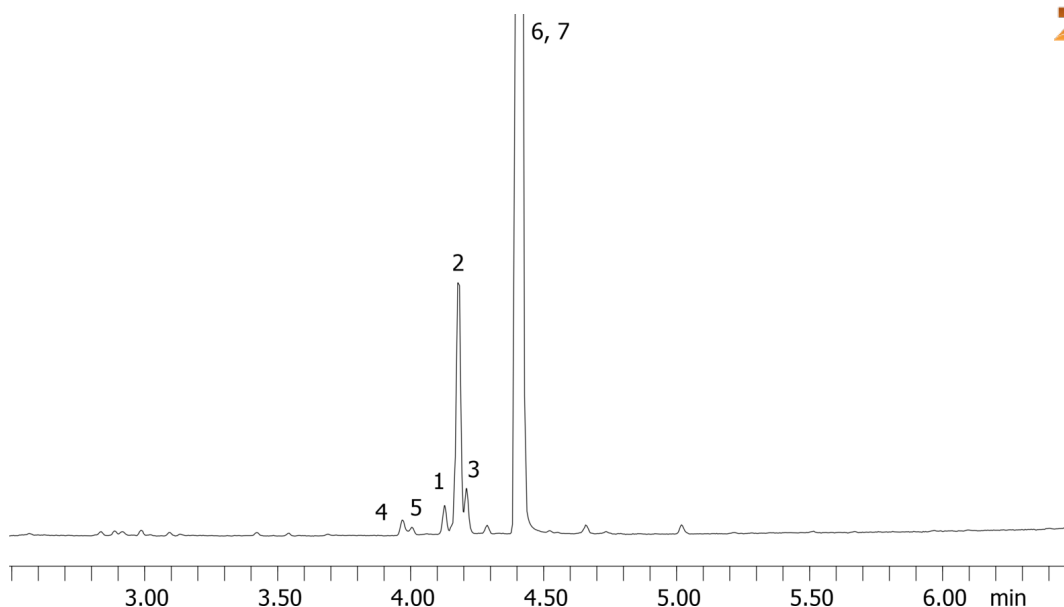