

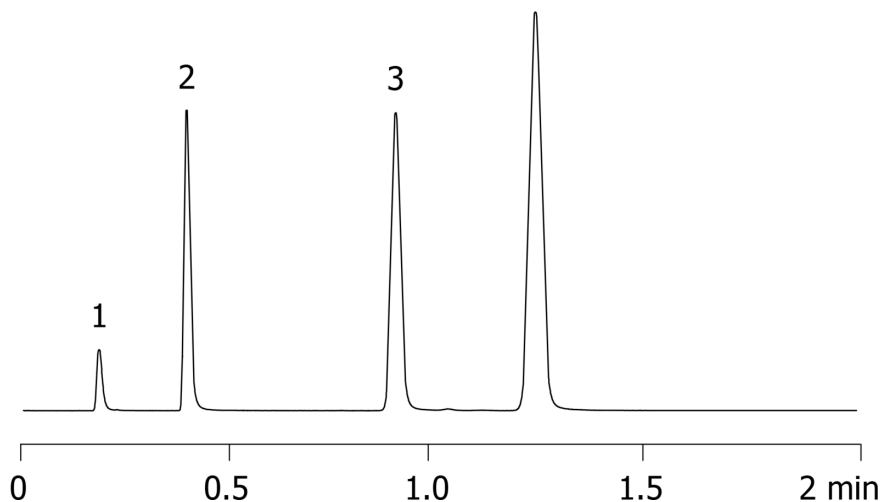
QC Test Chromatogram (Agilent 1200SL) - Kinetex 2.6µm C18 50 x 2.1mm ID**Column:** Kinetex® 2.6 µm C18 100 Å, LC Column 50 x 2.1 mm, Ea**Dimensions:** 50 x 2.1 mm ID**Order No:** 00B-4462-AN**Elution Type:** Isocratic**Eluent A:** Acetonitrile**Eluent B:** Water**Gradient**

Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	50	50

Flow Rate: 0.49 mL/min**Col. Temp.:** ambient**Detection:** UV-Vis Abs.-Variable Wave.(UV) @ 254 nm (ambient)

18566

4

**ANALYTES:****1** Uracil

Retention Time: 0.19 min

2 Acetophenone

Retention Time: 0.4 min

3 Toluene

Retention Time: 0.89 min

4 Naphthalene

Retention Time: 1.23 min

**Products used in this application:**