


**USP Glycerin Purity Assay on ZB-624****Column:** Zebtron<sup>TM</sup> ZB-624, GC Cap. Column 30 m x 0.53 mm x 3.00 µm, Ea**Phase:** 6% Cyanopropylphenyl 94% Dimethylpolysiloxane**Dimensions:** 30 meters x 0.53 mm x 3 µm**Order No:** 7HK-G005-36**Oven Profile:** 100 °C for 4 min to 120 °C @ 50 °C/min for 10 min to 220 °C @ 50 °C/min for 6 min**Carrier Gas:** Constant Flow Helium, 4.5 mL/min**Injection:** Split 10:1 1 µL @ 220°C**Detection:** Flame Ionization (FID) (250°C)**Analyst Note:** Concentrations were 2.0 mg/mL Glycerin, 0.050 mg/mL ethylene glycol, 0.050 mg/mL diethylene glycol, and 0.10 mg/mL 2,2,2-trichloroethanol (IS)**Products used in this application:**

19292

**ANALYTES:**

- 1 Ethylene glycol
- 2 2,2,2-Trichloroethanol
- 3 Diethylene glycol
- 4 Glycerin

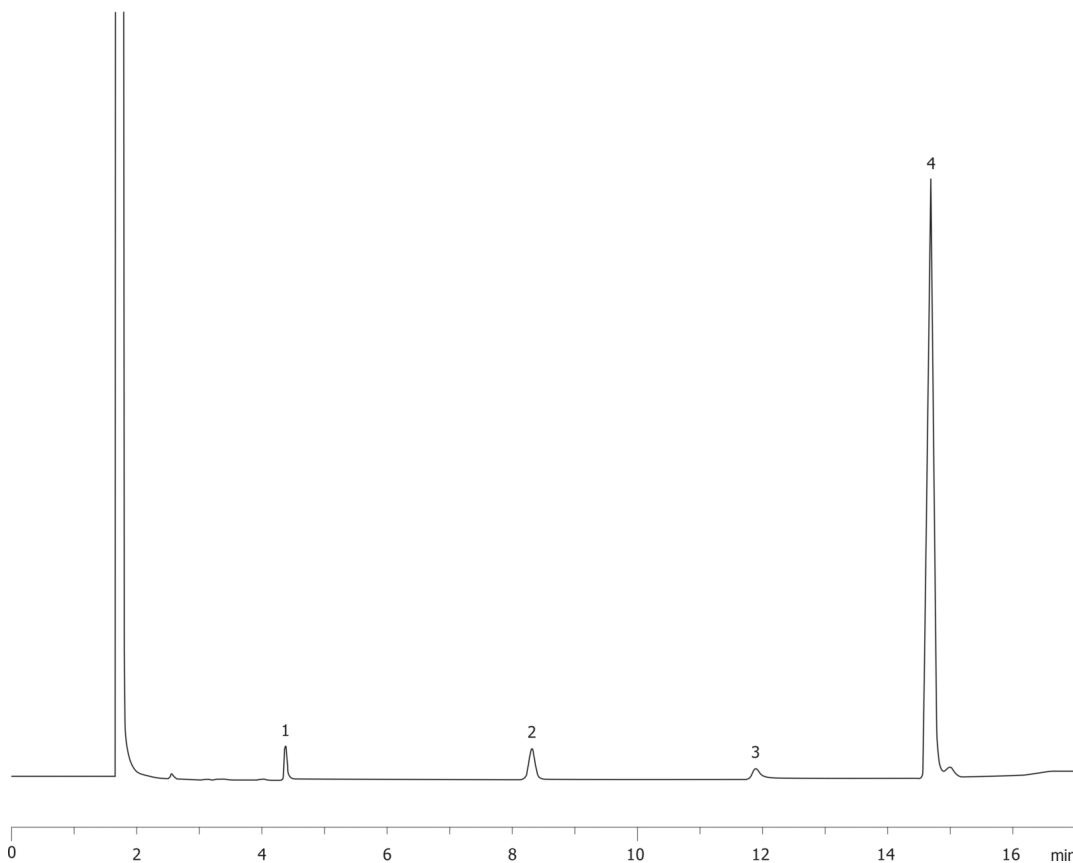