
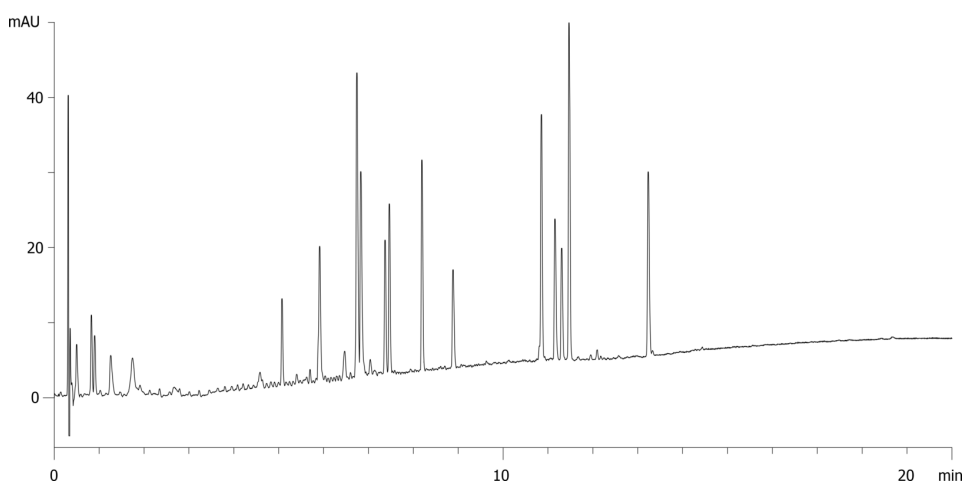


Hi Temp Stability - Injection on new Aeris WIDEPORE column**Column:** Aeris™ 3.6 µm WIDEPORE XB-C18 200 Å, LC Column 50 x 2.1 mm, Ea**Dimensions:** 50 x 2.1 mm ID**Order No:** 00B-4482-AN**Elution Type:** Gradient**Eluent A:** Water with 0.1% TFA**Eluent B:** Acetonitrile with 0.1% TFA

Gradient Profile:	Step No.	Time (min)	Pct A	Pct B
	1	0	97	3
	2	3	97	3
	3	23	35	65

Flow Rate: 0.312 mL/min**Col. Temp.:** 90 °C**Detection:** UV-Vis Abs.-Diode Array (PDA) @ 214 nm (ambient)**Analyst Note:** Application was actually run on a 50x4.6mm ID running at a flow rate of 1.5 mL/min. 50 x 4.6 mm which is not a commercially available part number. Information switched to 50x2.1mm for those that wish to replicate method.
AppID 19832**Products used in this application:****ANALYTES:****1** Apomyoglobin